

# INSTRUCTION MANUAL

# TALBOYS



Advanced High Speed Microplate Shaker

## TABLE OF CONTENTS

Package Contents	1
Warranty	1
Installation	2
Maintenance & Servicing	2
Environmental Conditions	2
Safety Instructions	3
Standards & Regulations	3
Specifications	4
Control Panel	5
Operating Instructions	6
Replacement Parts	7

### PACKAGE CONTENTS

Microplate Shaker  
92" (234cm) detachable power cord  
Instruction Manual  
Warranty card

### WARRANTY

Manufacturer warrants this product to be free from defects in material and workmanship when used under normal conditions for two (2) years. Please complete and return the enclosed warranty card. For your reference, make a note of the serial number, date of purchase and supplier here.

Serial No.: \_\_\_\_\_ Date of Purchase: \_\_\_\_\_

Supplier: \_\_\_\_\_

## **INSTALLATION**

---

1. **Important:** Choose the space on your bench where the Talboys High Speed Microplate Shaker will stay. Because of the amount of energy dissipated, the unit is held onto your lab bench with 12 rubber feet (suction cups). The unit is VERY difficult to remove from work surface and should be done with caution. Use paper under the feet to keep them from attaching to the bench while determining the final location. When final location is determined, remove the paper.
2. Be sure the power switch is in the off position.
3. The Talboys High Speed Microplate Shaker comes with a connector plug that is inserted into the IEC connector on the back of the unit first, then it can be plugged into a properly grounded outlet. The 120v unit plugs into a 120 volt, 50/60 Hz source. The 230v unit plugs into a 230 volt, 50/60 Hz source.
4. Your Talboys High Speed Microplate Shaker is ready for use.

## **MAINTENANCE & SERVICING**

---

The Talboys High Speed Microplate Shaker is built for long, trouble-free, dependable service. No lubrication or other technical user maintenance is required. It needs no user maintenance beyond keeping the surfaces clean. The unit should be given the care normally required for any electrical appliance. Avoid wetting or unnecessary exposure to fumes. Spills should be removed promptly. Do not use a cleaning agent or solvent on the front panel which is abrasive or harmful to plastics, nor one which is flammable. Always ensure the power is disconnected from the unit prior to any cleaning. If the unit ever requires service, contact your Talboys representative.

## **ENVIRONMENTAL CONDITIONS**

---

Operating Conditions: Indoor use only.

Temperature: 4 to 40°C (39.2 to 104°F)  
Humidity: 20% to 80% relative humidity, non-condensing  
Altitude: 0 to 6,562 ft (2000 M) above sea level

Non-Operating Storage:

Temperature: -20 to 65°C (-4 to 149°F)  
Humidity: 20% to 80% relative humidity, non-condensing

Installation Category II and Pollution Degree 2 in accordance with IEC 664.

## SAFETY INSTRUCTIONS

---

Please read the entire instruction manual before operating the unit.



**WARNING! DO NOT** use the **UNIT** in a hazardous atmosphere or with hazardous materials for which the unit was not designed. Also, the user should be aware that the protection provided by the equipment may be impaired if used with accessories not provided or recommended by the manufacturer, or used in a manner not specified by the manufacturer.

Always operate unit on a level surface for best performance and maximum safety.

**DO NOT** lift the Highspeed Microplate Shaker by the tray.



**CAUTION!** To avoid electrical shock, completely cut off power to the unit by disconnecting the power cord from the unit or unplug from the wall outlet. Disconnect unit from the power supply prior to maintenance and servicing.

Spills should be removed promptly

**DO NOT** immerse the unit for cleaning.

**DO NOT** operate the unit if it shows signs of electrical or mechanical damage.



Earth Ground - Protective Conductor Terminal

3

~ Alternating Current

## STANDARDS & REGULATIONS

---

Henry Troemner LLC hereby declares under its sole responsibility that the construction of this product conforms in accordance with the following standards:

### Safety standards:

IEC 61010-1 Safety requirements for electrical equipment for measurement, control and laboratory use. Part: I General Requirements.

IEC 61010-2-051 Part II: Particular requirements for laboratory equipment for mixing and stirring.

UL Std. No. 61010-1  
CSA/CAN C22.2

### EMC standards:

EN61326-1 Class A	EN61000-3-2
EN61000-4-5	EN61000-3-3
EN61000-4-4	EN61000-4-2
EN61000-4-3	EN61000-4-11
EN61000-4-6	EN61000-4-8


### Associated EU guidelines:

EMC directive 89/336/EEC  
LVD directive 73/23/EEC

## SPECIFICATIONS - HIGH SPEED MICROPLATE SHAKER



<b>Overall dimensions (L x W x H):</b>	15.5 x 12 x 12.8" (39.4 x 30.5 x 32.5cm)
<b>Tray dimensions (L x W):</b>	12.25 x 11" (31.1 x 27.9cm)
<b>Electrical (50/60 Hz):</b>	120 V - 1 amps, 120 watts 230 V - 1 amp, 120 watts
<b>Fuses:</b>	5mm x 20mm, 5 amp quick acting (2 required)
<b>Speed range:</b>	600 to 2500rpm
<b>Timer:</b>	1 second to 160 hrs
<b>Orbit:</b>	.014" (3.6mm)
<b>Controls:</b>	See page 5
<b>Ship weight:</b>	50lbs (22.7kg)
<b>Capacity:</b>	7 lbs (3.2kg) 48 microplates in stacks up to 5" high

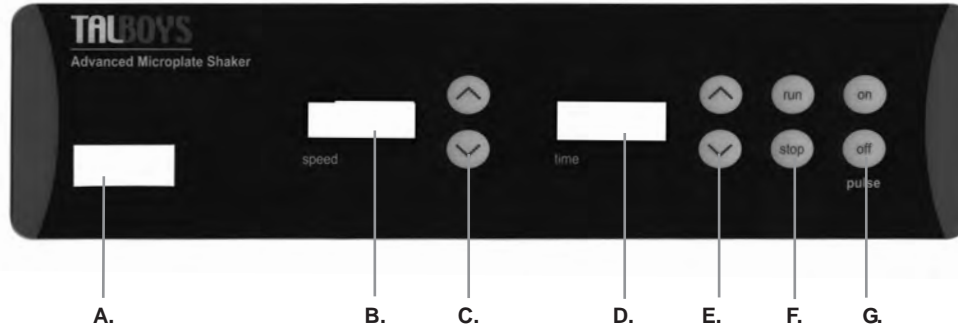

## CONTROL PANEL - HIGH SPEED MICROPLATE SHAKER

The front panel of the High Speed Microplate Shaker contains all the switches, controls and displays needed to operate the unit.

**A. On/off rocker switch:** Turns main power on/off.

**B. Speed display:** Displays the speed of the shaker.

**C.** Up/down arrows for set-point control.

**D. Time display:** Displays accumulated time (continuous mode) or how much time is remaining (timed mode). The display range is from 0 to 9,999 minutes in one (1) second increments. The display will indicate minutes and seconds until the timer reaches 99 minutes and 59 seconds (99:59), then the display will automatically display minutes up to 9,999.

**E.** Up/down arrows for set-point control.

**F. Run/stop buttons:** Activates shaking.

**G. Pulse on/off buttons:** Activates pulse mode.

## **OPERATING INSTRUCTIONS**

---

1. Flip up the four quick release latches which will release top tray from the 4 posts. DO NOT USE without both top and bottom tray foam in place.
2. Your Digital High Speed Micro Plate Shaker is designed to hold up to 7 pounds, which will accommodate deepwell blocks or stacked microplates up to 5" high.

**To avoid excessive noise and potential block damage, well blocks should always have space between them and should never touch each other.**

3. Sample containers should be placed on bottom tray foam insert and centered on the tray to achieve optimal performance.
4. To place top tray on unit, place the short side to the front engaging the 4 posts. When top tray is lined up, press down on the center of the tray and engage by pushing the quick release latches down into the locked position. Repeat for all corners. When top plate is locked in place, tighten the knobs on the four adjustment blocks. The High Speed Micro Plate Shaker is ready to operate. When changing samples, disengage the four quick release latches to remove the top tray. Do not loosen the knobs on the adjustment blocks. Loosen and move the four adjustment blocks only when the sample heights have changed.
5. Turn the Power on by depressing the left side of the rocker switch on the bottom left side of the control panel. LED displays for Speed and Timer will light.
6. Set speed by pressing the up/down arrows to the right of the speed display until you reach the desired speed. Adjust Time using the up/down arrows to the right of the timer display. Press the run button. The unit will run for the programmed time. Timer

LED will display time remaining.

7. To run in the un-timed mode, set the time to zero (0) using the up/down arrows to the right of the timer display. Press the run button and the unit will run until you press the stop button. Timer LED will display accumulated time.
8. To run in pulse mode unit must not be running. Press the "ON" button above the word "PULSE". To stop the pulse feature press the "OFF" button above the word "PULSE". Pulse mode is factory programmed for 2 seconds on 1 second off. The pulse "ON" and pulse "OFF" times can be adjusted between 1 and 59 seconds in 1 second intervals.

**The Pulse time can be reprogrammed by following the directions below.**

### **Pulse "ON" time**

- a. Turn power off
- b. Turn power on while holding pulse "ON" button. The LED display for "SPEED" shows current pulse on time.
- c. Change the pulse on time using the up/ down arrows to the right of the "SPEED" display.
- d. When the power is turned off, the value on the display is stored as the new pulse on time.

### **Pulse "OFF" time**

- a. Turn power off
- b. Turn power on while holding pulse "OFF" button. The LED display for "TIMER" shows current pulse off time.
- c. Change the pulse off time using the up/down arrows to the right of the "TIMER" display.
- d. When the power is turned off, the value on the display is stored as the new pulse off time.

## REPLACEMENT PARTS

---

DESCRIPTION	PART NUMBER
Top Tray	945177
Bottom Tray	245070-00
Motor	380006-00
Front Panel Membrane Switch	545044-00
Top Cover Motor	245030-00
Power Entry Module, 120V	380506-00
Power Entry Module, 230V	380237-00
Transformer, 230V	380700-00
Processor Board	345103-00
Feet	545014-00
Rocker Switch	380008-00
Knob	545035-00
Tray Pad Set	945176
Detachable 92" (234cm) Power Cord: 120V	330100-00
Euro	330101-00
UK	330102-00
Swiss	330103-00

---

MANUFACTURED BY:

### HENRY TROEMNER LLC

201 Wolf Drive • PO Box 87 • Thorofare, NJ 08086-0087  
Phone: 856-686-1600 • Fax: 856-686-1601 • E-mail: [troemner@troemner.com](mailto:troemner@troemner.com)  
[www.troemner.com](http://www.troemner.com)